

Item Catalogue

NUPCO CODE: 4224210003500 | SN: 1331

NUPCO ITEM DESCRIPTION

PLATE, LCP ANATOMIC CRONOID PLATING, TITANIUM, ASSORTED TYPES AND SIZES REQUESTED BY END USER

VENDOR PRODUCT DESCRIPTION

Elbow Plating System coronoid plates

SKU CODES INCLUDED FOR THIS NUPCO CODE

- 70-0413
- 70-0414
- 70-0415
- 70-0416



Surgical Technique



Coronoid Plates Surgical Technique

Shawn W. O'Driscoll, MD, PhD



Figure 36

1 Fracture Fragment Fixation

Expose the coronoid and ridge of the ulna through an anteromedial approach. Reduce and provisionally hold the fragments with smooth .045" x 6" ST Guide Wires (WS-1106ST) functioning as K-wires.



Figure 37

2 Plate Placement and Provisional Fixation

Apply the Coronoid Plate (70-041X) so that the two prongs on the proximal section grasp and buttress the anteromedial facet of the coronoid. If the sublime tubercle, on which the anterior bundle of the medial collateral ligament (MCL) inserts, is also fractured (Anteromedial Subtype III fracture), the offset screw hole should sit over that fragment for proper screw position. The distal portion of the plate should extend along the ridge on the anteromedial side of the ulna. Several .045" K-wires may be used for provisional plate fixation through the K-wire holes in the plate.

Note: Use caution when handling the plate as it has sharp prongs. Repeated and excessive bending may damage the plate, causing it to not fit or function as intended.

Note: Plates designed for use on the left arm are blue. Plates designed for use on the right arm are green.

Screw Diameter	Drill Diameter
2.7 mm	2.0 mm

Coronoid Plates Surgical Technique [continued]

Figure 38



3 Initial Central Nonlocking Screw

The first screw inserted is a 2.7 mm Nonlocking Hexalobe Screw (30-03XX) or 2.7 mm Nonlocking Hexalobe CoCr Screw (3061-270XX) into hole #1, which is the “central” plate hole. Drill using the 2.0 mm Quick Release Drill (80-0318) and measure for the screw length using the Depth Gauge 6–65 mm (80-0623). Connect the T8 Stick Fit Hexalobe Driver (80-0759) to the Medium Ratcheting Driver Handle (80-0663) and insert the screw. When determining the screw lengths, make sure to compensate for any expected plate deformation if the bend does not fully seat the plate against the bone. As the screw is tightened, the plate will flex and contour to the bone. If the outer proximal hole begins to bend outward, tighten this first screw only partially, insert the most proximal screw, then go back to fully seat the central screw. Seating this screw may also cause the prongs on the proximal portion of the plate to buttress the coronoid and further compress the plate to the bone.

Note: Tapping the bone prior to screw insertion with the Bone Tap for 2.7 mm Hexalobe Screws (80-0625) may be needed for patients with dense bone (see Tapping Instructions on page 21).

Figure 39



4 Coronoid Fixation

To fill the proximal 2.7 mm nonlocking hexalobe screw holes (holes #2 and #3), use the same technique as in Step 3. The offset screw hole, #4, is optional and can be filled with a nonlocking screw if the fracture extends to the sublime tubercle. As these nonlocking screws are inserted, the plate will continue to contour to the bone.

Note: If K-wires were inserted for provisional fixation, they should be removed prior to drilling and inserting screws into the proximal portion of the plate.

Note: Use of fluoroscopy is recommended to verify the trajectory of the nonlocking screws to ensure they avoid the articular surface.

Coronoid Plates Surgical Technique [continued]



Figure 40

5 Insert Remaining Locking Screws

To insert the 2.7 mm Locking Hexalobe Screws (30-03XX) or 2.7 mm Locking Hexalobe CoCr Screws (3060-270XX), thread the 2.0 mm Locking Drill Guide (80-0621) into each distal plate hole (#5 and #6) and drill with the 2.0 mm Quick Release Drill (80-0318). Insert the locking screws with the T8 Stick Fit Hexalobe Driver (80-0759) and the Medium Ratcheting Driver Handle (80-0663). Nonlocking screws can be used at the surgeon's discretion.

Note: Care should be taken not to overtighten the screws or apply excess torque on the driver.



Figure 41

6 Postoperative Protocol

Note: The following protocol may be replaced with an alternative protocol at the performing surgeon's discretion.


Immediately after closure, the elbow is placed in a bulky noncompressive Jones dressing with an anterior plaster slab to maintain the elbow in a relatively extended position and the upper extremity is kept elevated for three days, bringing it down from the elevated position each hour for 5–10 minutes to permit adequate perfusion. The initial rehabilitation is planned according to the stability of the elbow, the security of fracture fixation, and the extent of soft-tissue damage.

7 Optional: Implant Removal Instructions

To remove a Coronoid Plate, use a T8 Stick Fit Hexalobe Driver (80-0759) and a Quick Release T-Handle (MS-T1212) to remove all screws before extracting the plate. Referencing the Screw Removal Brochure (SPF10-00) may aid in implant extraction if difficulty is experienced.

Caution: 2.7 mm Hexalobe locking & nonlocking CoCr screws (3060-270XX, 3062-350XX); (3061-270XX, 3063-350XX) are not compatible with Acumed Screw Removal system.

Ordering Information [continued]

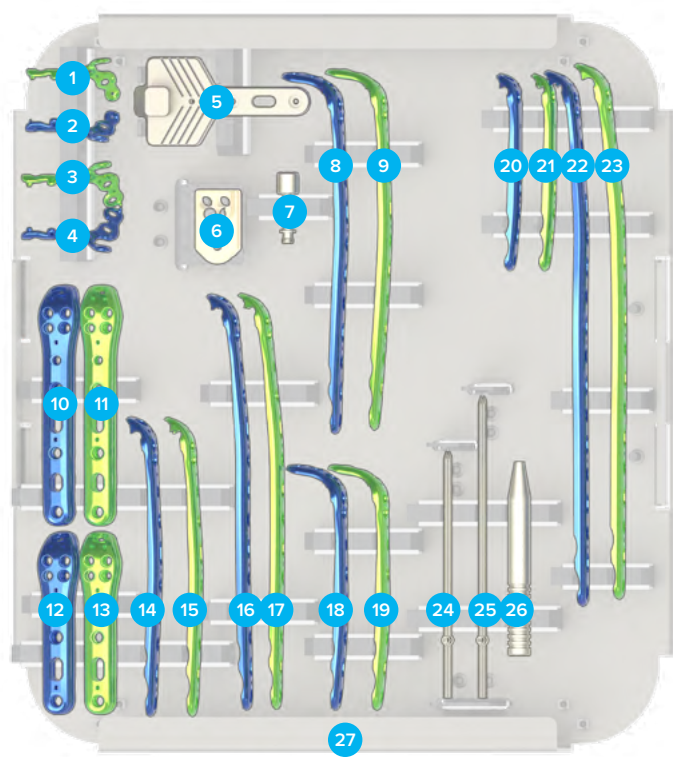

Tray Components

Coronoid Plates

3	Coronoid Plate, Standard, Right	70-0414
4	Coronoid Plate, Standard, Left	70-0413

Instrumentation

5	Olecranon Plate Osteotomy Cutting Jig	80-0653
6	Olecranon Plate Prox Targeting Guide	80-0654
7	Locking Bolt: M4	80-0652

Olecranon Plates

8	Olecranon Plate, Extended, 9-hole, Left (130 mm)	70-0314
9	Olecranon Plate, Extended, 9-hole, Right (130 mm)	70-0315
10	Olecranon Plate, Standard, 5-hole, Left (90 mm)	70-0304
11	Olecranon Plate, Standard, 5-hole, Right (90 mm)	70-0305
12	Olecranon Plate, Standard, 3-hole, Left (65 mm)	70-0302

Tray Components

13	Olecranon Plate, Standard, 3-hole, Right (65 mm)	70-0303
14	Olecranon Plate, Standard, 7-hole, Left (110 mm)	70-0306
15	Olecranon Plate, Standard, 7-hole, Right (110 mm)	70-0307
16	Olecranon Plate, Standard, 11-hole, Left (150 mm)	70-0308
17	Olecranon Plate, Standard, 11-hole, Right (150 mm)	70-0309
18	Olecranon Plate, Extended, 5-hole, Left (90 mm)	70-0312
19	Olecranon Plate, Extended, 5-hole, Right (90 mm)	70-0313

Instrumentation

24	70 mm Tension Band Pin	30-0098
25	90 mm Tension Band Pin	30-0099
26	Tension Band Pin Snapper	80-0411
27	Elbow System Olecranon-Coronoid Platter	80-0677

Optional Components from Elbow Plating System

Coronoid Plates

1	Coronoid Plate, Small, Right	70-0416
2	Coronoid Plate, Small, Left	70-0415

Olecranon Plates

20	Olecranon Plate, Narrow, 5-hole, Left (85 mm)	70-0316
21	Olecranon Plate, Narrow, 5-hole, Right (85 mm)	70-0317
22	Olecranon Plate, Standard, 15-hole, Left (190 mm)	70-0310
23	Olecranon Plate, Standard, 15-hole, Right (190 mm)	70-0311